

EDINBURGH
ANALYTICAL



DB30 DOUBLE BEAM UV-VIS SPECTROPHOTOMETER

EXCELLENCE IN SPECTROSCOPY PRECISION IN EVERY MEASUREMENT


EDINBURGH ANALYTICAL

Edinburgh Analytical provides cutting-edge solutions and support for general and analytical laboratories while maintaining the core values and culture of excellence that define Edinburgh Instruments.

EDINBURGH INSTRUMENTS

Edinburgh Instruments has been providing high performance molecular spectroscopy instrumentation for over 50 years.

Our photoluminescence, Raman, and transient absorption spectrometers set the standard in advanced optical spectrometers for research and industry.

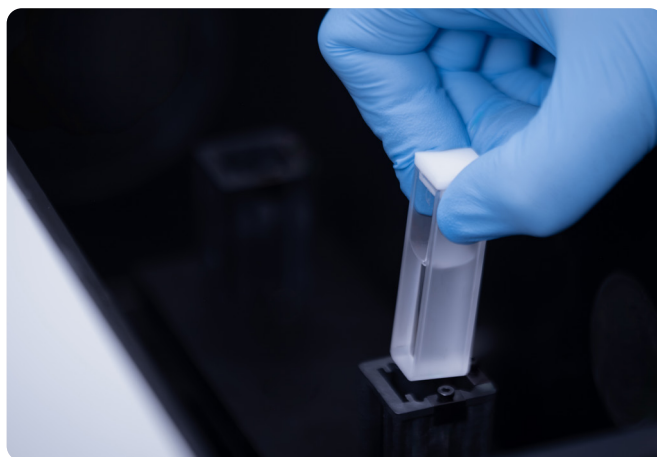

DB30 APPLICATIONS



Pharmaceuticals



Food



Molecular Biology



Chemistry



Life Sciences




Environmental




Petrochemical

MOLECULAR SPECTROSCOPY | UV-Vis | FTIR | Fluorescence



INTRODUCING DB30 HIGH PERFORMANCE DOUBLE BEAM UV-VIS SPECTROPHOTOMETER

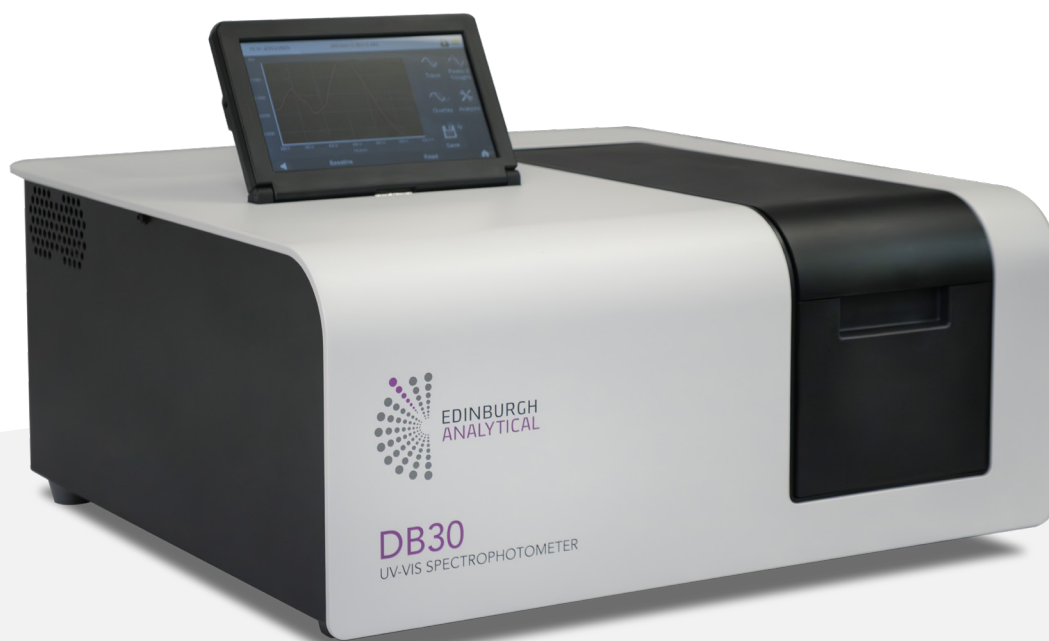

The DB30 UV-Vis Spectrophotometer is a high performance double beam instrument suitable for many analytical applications where accurate measurements are key to your results.

The DB30 measures absorption and transmission as a function of wavelength and provides a modern, user-friendly and accurate spectrophotometer for a wide range of sample types and measurements.


Utilising a dual lamp and Czerny-Turner configuration monochromator, the DB30 features a compact, reliable and high throughput optical system which ensures impressive spectral performance. It can be configured with PC control software or as a standalone instrument using the touchscreen included in every DB30 unit.



KEY FEATURES

- > User selectable variable bandpass at 0.5, 1.0, 1.5, 2.0 or 4.0 nm
- > Fast scanning – up to 6,000 nm/min for high sample analysis throughput
- > Automatic accessory recognition
- > Modern touchscreen interface for full standalone control
- > Optional Visacle® software for PC control
- > USB, SD card and internal data storage for convenient retrieval of methods and results

SAMPLE ACCESSORIES



STANDARD CELL HOLDER

The standard cell holder is 2-position and holds traditional 10 mm path length cells. A micro-volume cell holder option for 50 μ l cells is also available.




LONG PATH CELL HOLDER

Designed for low concentrations or absorbance, the long path cell holder holds two rectangular cells with an optical path length of 10 mm to 100 mm.



GLASS FILTER HOLDER

Designed for measuring the transmittance/absorbance of glass samples or filters. Sample dimensions up to 55 mm x 100 mm with 5 mm thickness can be accepted.



FILM HOLDER

Designed for measuring the transmittance/absorbance of thin-film samples. Sample dimensions up to 25 mm x 50 mm can be measured.



THERMOSTATIC CELL HOLDER

Designed for incubation or temperature stabilisation from room temperature to +40°C. Temperature stability $\pm 0.3^\circ\text{C}$.



6-POSITION CELL HOLDER

Mount up to 6 standard 10 mm path length cells with auto-changeover of sample.



AUTO SIPPER

Designed for rapid and automatic measurement of multiple or large amounts of liquid sample without changing cells.



MICRO FLOW CELL

Designed for continuous measurement of trace samples. Flow cell capacity of 70 μ l, 10 mm path length with Teflon tubing.



ELECTRONIC TEMPERATURE CONTROLLED CELL HOLDER

Designed for precise temperature control measurement.

Name	Description
Standard Cell Holder	2-position cell holder for standard 10 mm cells
Thermostatic Cell Holder	Thermostatic cell holder with temperature control from room temperature up to +40°C
Long Path Cell Holder	Holds two rectangular cells with an optical path length of 10 mm to 100 mm
Glass Filter Holder	Holds glass samples/filters for transmittance/absorbance measurements
Film Holder	Holds thin-film samples for transmittance/absorbance measurements
6-Position Cell Holder	Holds up to six 10 mm cells in a carousel with auto-rotation into the sample beam
Auto Sipper	For multiple or large amounts of liquid samples without manual washing or changing of cells
Micro Flow Cell	Continuous measurement by injection with syringe or other device for volumes up to 70 μ l
Micro Cell Holder	Holds micro cells for measuring micro-volumes of 50 μ l
Electronic Temperature-Controlled Cell Holder	Electronic temperature-controlled cell holder for precise control from 15°C to 110°C and built-in stirring

INSTRUMENT CONTROL

CHOOSE BETWEEN TOUCHSCREEN OR SOFTWARE OPERATION

The DB30 can be operated via a touchscreen that is included with every DB30. Optional Visacle® PC-control software is available for laboratories wishing to control their instrument from a computer or manage their experiment database. FDA 21 CFR Part 11 compliance is also available as an option.




TOUCHSCREEN OPERATION

MEASUREMENT MODES

- > **Wavelength scan:** Measure absorbance, transmission or detector signal selecting the spectral range, scan speed, wavelength increment, bandwidth as well as advanced instrumental parameters
- > **Time scan:** Perform kinetic measurements for time periods ranging from 1 minute to >27 hours
- > **Photometry mode:** Multiple wavelengths measurement in either absorbance or transmittance modes, from single up to 10 different individual wavelengths
- > **Quantitation:** Calibration curves including second order and multi-wavelength data points
- > **Application wizards:** Protein, nucleic acid, hexavalent chromium

DATA HANDLING

- > Rescaling, data readout, spectrum overlay, peak & trough analysis, arithmetic, smoothing, differentiation, area & rate calculating
- > Report generation and file output in CSV format
- > Internal memory, external USB, SD card

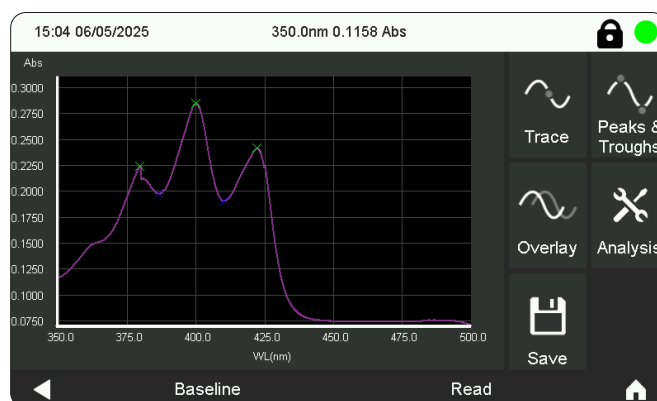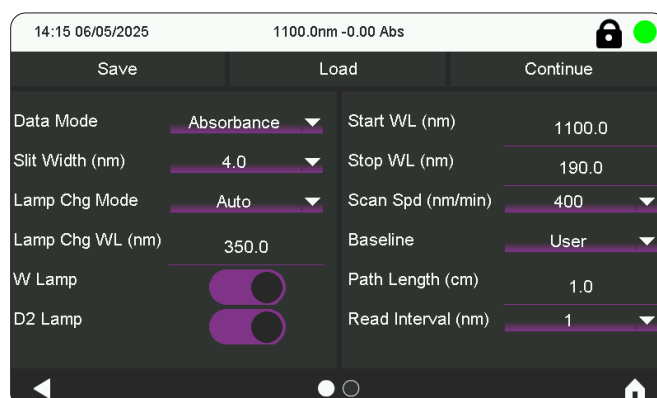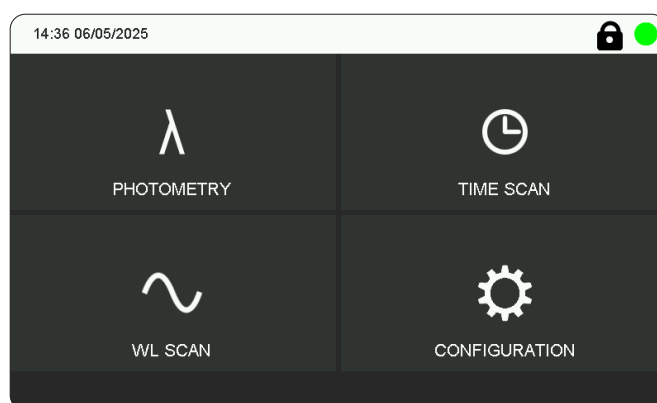

Measurement parameters, acquisition and analysis on DB30 touchscreen



USER FRIENDLY SOFTWARE

VISACLE® PC-CONTROLLED SOFTWARE

Visacle® offers all control, validation, data analysis and reporting functionality for DB30 in one PC-operated software package. Collected data is stored in a secure database, where it can then be organised and analysed, as well as exported in .TXT, .CSV or PDF format. Visacle® can be purchased as a CFR Part 11 compliant package for users requiring additional security.

Visacle-CFR features include:

- > Configurable user profiles with secure login and e-signatures
- > Audit trail logging of all actions taken
- > Permission system to restrict actions and data access to authorised users



Project browser

Name	Author	Date Created	Date Modified	Method Type	Notes
Default	Edinburgh Instruments	26/03/2025 14:54	06/05/2025 13:...		Pre generated common meth...
Methods					
<input checked="" type="checkbox"/> New Method 20250506 1341	Unknown	06/05/2025 13:41	16/05/2025...	Wavelength	
<input type="checkbox"/> New Method 20250502 1031	Unknown	02/05/2025 10:31	02/05/2025...	Quantitation	
<input type="checkbox"/> New Method 20250502 1026	Unknown	02/05/2025 10:26	02/05/2025...	Quantitation	
<input type="checkbox"/> New Method 20250501 1432	Unknown	01/05/2025 14:35	01/05/2025...	Time	
<input type="checkbox"/> New Method 20250501 1431	Unknown	01/05/2025 14:31	01/05/2025...	Quantitation	
<input type="checkbox"/> New Method 20250501 1431	Unknown	01/05/2025 14:31	01/05/2025...	Time	
<input type="checkbox"/> New Method 20250501 1407	Unknown	01/05/2025 14:07	01/05/2025...	Wavelength	
<input type="checkbox"/> New Method 20250428 1337	Unknown	28/04/2025 13:38	28/04/2025...	Wavelength	
<input type="checkbox"/> New Method 20250327 1604	Unknown	27/03/2025 16:04	27/03/2025...	Wavelength	
<input type="checkbox"/> New Method 20250326 1454	Unknown	26/03/2025 14:54	26/03/2025...	Wavelength	
Amino Acridine Photometry	Edinburgh Instruments	26/03/2025 14:54	26/03/2025...	Photometry	
Amino Acridine Quantitation	Edinburgh Instruments	26/03/2025 14:54	26/03/2025...	Quantitation	
Amino Acridine Time	Edinburgh Instruments	26/03/2025 14:54	26/03/2025...	Time	
Amino Acridine Wavelength	Edinburgh Instruments	26/03/2025 14:54	26/03/2025...	Wavelength	
Sample groups					
<input checked="" type="checkbox"/> Lab1	WY	16/05/2025 10:55	16/05/2025...	Wavelength	
<input checked="" type="checkbox"/> Annual check	WY	16/05/2025 10:51	16/05/2025...	Wavelength	
<input checked="" type="checkbox"/> SampleGroup Wavelength	Unknown	06/05/2025 13:42	06/05/2025...	Wavelength	

Visacle® spectral acquisition interface and CFR project browser



SPECIFICATIONS

DB30 UV-Vis Spectrophotometer

Working Environment and Requirements

Working Temp 10 - 35°C ambient temperature

Power Supply 100-240 V, 50-60 Hz

Main Specifications

Optics Czerny-Turner, double beam monochromator

Wavelength Range 190 nm – 1,100 nm

Spectral Bandwidth 0.5 nm, 1 nm, 1.5 nm, 2 nm and 4 nm

Stray Light $\leq 1\%$ (198 nm KCl), $\leq 0.05\%$ (220 nm NaI, 340 nm NaNO₂)

Wavelength Accuracy ± 0.1 nm at D2 peak 656.1 nm, ± 0.25 nm entire range

Wavelength Repeatability ≤ 0.1 nm (max deviation), ≤ 0.05 nm (standard deviation)

Photometric Range Absorbance: -3.4 to +3.4, %T: 0 to 300, Concentration: 0.000 to 9,999

Photometric Accuracy ± 0.002 Abs (0 - 0.5 Abs), ± 0.004 Abs (0.5 - 1.0 Abs), ± 0.008 Abs (1.0 - 2.0 Abs), $\pm 0.3\%$ T

Photometric Reproducibility ± 0.0005 Abs (0.5 Abs), ± 0.001 Abs (1.0 Abs), ± 0.004 Abs (2.0 Abs)

Wavelength Scan Speed 10, 100, 200, 400, 800, 1200, 2400, 3600, 6000 nm/min

Noise 0.0001 Abs (peak-to-peak) 0.00005 Abs (RMS)

Baseline Stability 0.0003 Abs/hr (500 nm, 2 hour lamp warm-up period)

Baseline Flatness ± 0.0009 Abs (200 nm - 950 nm)

Light Source Tungsten-halogen and deuterium lamps

Light Source Switching Automatic switching selectable for 325 nm - 370 nm range

Detector Silicon photodiode

Display 7" touchscreen

Software Touchscreen operation, PC-controlled software or CFR compliant PC-controlled software

Dimension (LxDxH) 500 mm (W) × 475 mm (D) × 250 mm (H)

Net Weight 20 kg (approx)

Output Device USB flash drive, SD card

Interface USB PC interface

Scope of delivery

Box includes
1 x DB30 Unit
1 x Operation Manual
2 x Quartz Cuvette

After Sales Service

Warranty Guaranteed (under normal maintenance) for one year from the date of delivery



EDINBURGH
ANALYTICAL



SCAN ME

EDINBURGH ANALYTICAL

2 Bain Square, Livingston, EH54 7DQ, United Kingdom

Tel: +44 (0)1506 425 300

Fax: +44 (0)1506 425 320

sales@edinst.com

Registered in England and Wales No: 962331 VAT No:GB 271 7379 37

©Edinburgh Instruments Ltd 2026

STG08 / 05.2026



Customer support is available worldwide

www.edinburghanalytical.com

